


## Intensity Distribution with a cutoff of $-3.74$

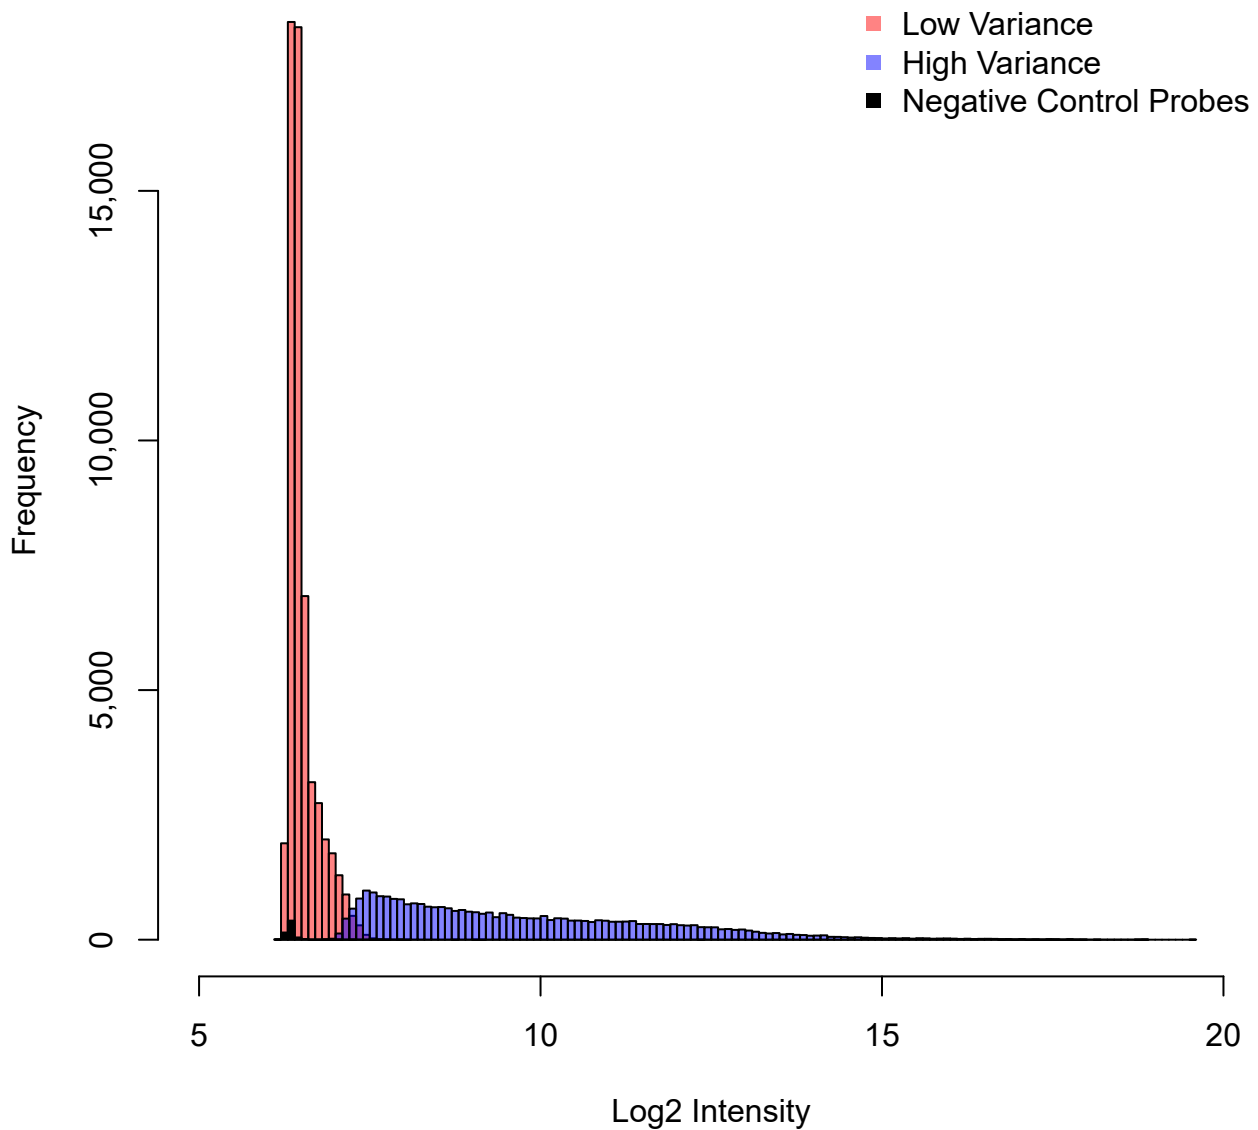

### Supplemental Figure SF2

Distribution of the log<sub>2</sub> intensity values of probes with a log variance respectively below (low variance probes) and above (high variance probes) the cutoff of  $-3.74$ , and of the negative control probes.